
ISO-TECH DIGITAL LIGHT METER

LUX-1335 INSTRUCTION MANUAL

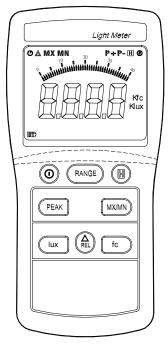

INTRODUCTION

- The ISO-TECH LUX-1335 digital light meter is a precision instrument used to measure illuminance (lux, footcandle).
- It meets CIE photopic spectral response.
- It is fully cosine corrected for the angular incidence of light.
- The meter is a compact, tough and easy to use instrument.
- The light sensitive component used in the meter is a very stable, long-life silicon photodiode and spectral response filter.
- U.S. Pat. No. Des. 446,135

II FEATURES

- Light measurement ranging from 0.01 lux ~ 0.1 klux / 0.01 fc ~ 0.01 kfc, respectievely.
- High accuracy and rapid response.
- Data-hold function
- Digital and analogue graphical display
- Automatic zeroing.
- Meter corrected for spectral relative efficiency.
- No manual correction factor calculations for non-standard light sources.

1


- Short rise and fall times.
- Peak-hold function
- Selectable scale Lux or fc
- Auto power off after 30 minutes.
- Maximum and minimum measurements.
- Relative reading function.

IV METER DIAGRAM

III SPECIFICATIONS

- Display : 3-3/4 digit LCD with high speed 42 segment bargraph.
- Measuring Range : 40.00 lux, 400.0 lux, 4000 lux, 40.00 klux and 200.0 klux / 40.00 fc, 400.0 fc, 4000 fc, 20.00 kfc. Note : 1fc=10.76Lux , 1lux=1000Lux , 1kfc=1000fc
- Overrange Display : LCD will show "OL" symbol.
- Spectral Response : CIE Photopic. (CIE human eye response curve).
- Spectral Accuracy : CIE V λ function f '₁ \leq 6%
- Accuracy: ±3% rdg ± 0.5% f.s. (±4% rdg±10 dgts as > 10,000 lux/fc range).
 (calibrated to standard incandescent lamp at colour
- (calibrated to standard incandescent lamp at colour temperature 2856 K) .
- Repeatability : ±2% .
- Temperature Characteristics : ±0.1%/°C.
- Sampling Rate : 13.3 times/sec for analogue bar-graph indication ; 1.3 times/sec for digital display.
- Photo Detector : Silicon photo diode and spectral response filter.
- Operating Temperature & Humidity : $0^\circ\!C$ to $40^\circ\!C~(32^\circ\!F$ to $104^\circ\!F\,)$ & 0% to 80% RH.
- Storage Temperature and Humidity : -10 $^\circ\!C$ to 50 $^\circ\!C$ (14 $^\circ\!F$ to 140 $^\circ\!F$) & 0% to 70% RH.
- Power Source : 6 x 1.5V AAA batteries
- Battery life (typical) : 400 hours (zinc-carbon).
- Photo detector Lead Length : 150 cm (approx.).
- Photo detector Dimensions : $92L \times 60W \times 29H$ (mm);
- Meter Dimensions : 150L × 72W × 35H (mm);
- Weight : 320g .
- Accessories : Carry case & instruction manual



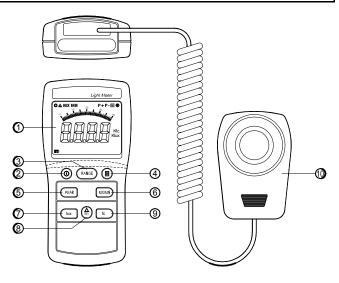

- 1. LCD Display : 3-3/4 digit display with a maximum reading of 3999, and the indicating signs of measured values, unit function symbols, and decimal points etc are displayed.
- 2. ON/OFF button.
- Range Selector button: Sequential selection of 40.00 lux, 400.0 lux, 4000 lux, 40.00 Klux 200.0 klux or 40.00 fc, 400.0 fc, 4000 fc, 20.00 Kfc. Total of 5 range for lux and 4 range for fc.
- 4. Data-Hold button
- 5. Peak Hold button

- 6. MX/MN button: Maximum and Minimum reading recall
- 7. Lux button : Pressing the Lux button selects taking measurement of illuminance in lux.
- 8. Relative Reading button
- 9. fc button : Pressing the fc button selects measurement of illuminance in footcandle scale; and, 1 footcandle = 10.76 lux.

10. Photo Detector.

V OPERATING INSTRUCTIONS

- 1. Power-up : Press the power button to turn the meter ON or OFF.
- 2. Selecting the lux or fc scale : Set the range selection switch to desired lux or fc range.
- 3. Remove the photo detector cap and hold the sensor towards the light source in a horizontal position.
- 5. Overange : If "OL" is shown on the display, the input signal is too strong and a higher range should be selected.
- Data-Hold mode : Press the HOLD button to select Data-Hold mode. When HOLD mode is selected, the illuminance meter stops all further measurements. Press the HOLD button again to exit DATA-HOLD mode and continue taking readings
- Peak-Hold recorder mode : Press and hold down PEAK button until the display shows "CAL". Press the PEAK button repeatedly to reach P+ and P- mode as required. Expose the photo detector to the pulsating light field and read the result. Press and hold down PEAK button for 2 seconds to exit PEAK recorder mode, then the meter will resume normal operation.
 - 4


- Maximum and Minimum record mode : Press MX/MN button to cycle through Maximum (MX) reading, Minimum (MN) reading and current reading (MX/MN blink) recorder mode. Press MX/MN button for two seconds to exit this mode.
- 10. When the measurement is completed, replace the photo detector cap and turn the meter off.

VI BATTERY CHECK & REPLACEMENT

- 1. If the battery power is low, the LCD will display "BT" and battery replacement is required.
- 2. After turning off the meter, press the battery cover and push in the direction of the arrow to open.
- 3. Remove the batteries from the instrument and replace with 6 x 1.5V AAA batteries.
- 4. Replace cover.

VII SPECTRAL SENSITIVITY CHARACTERISTICS

• The response of the photo diode with the filters gives a spectral sensitivity characteristic of the meter which almost matches the C.I.E. (INTERNATIONAL COMMISSION ON ILLUMINATION) photopic curve V(λ) as shown in the following chart.



VIII MAINTENANCE

5

- 2. Do not store the instrument where temperature or humidity is excessively high.
- 3. The reference level, as marked on the face plate, is the tip of the photo detector globe.
- 4. The calibration interval for the photo detector will vary according to operational conditions, but generally the sensitivity decreases in direct proportion to the product of luminous intensity and the operational time. In order to maintain the basic accuracy of the instrument, periodic calibration is recommended.

IX RECOMMENDED ILLUMINATION			
1fc = 10.76 Lux			
LOCATIONS	Lux	fc	
 OFFICE Conference, Reception room. Clerical work Typing drafting 	200 ~ 750 700 ~ 1,500 1000 ~ 2,000	18 ~ 70 65 ~ 140 93 ~ 186	
 FACTORY Visual work at production line Inspection work Electronic parts assembly line Packing work, Entrance passage 	300 ~ 750 750 ~ 1,500 1500 ~ 3,000 150 ~ 300	28 ~ 70 70 ~ 140 140 ~ 279 14 ~ 28	

6

•	HOTELS Public room, Cloakroom Reception Cashier	100 ~ 200 200 ~ 500 750 ~ 1000	9 ~ 18 18 ~ 47 70 ~ 93
•	STORES Indoors Stairs Corridor Shop window, Packing table Forefront of shop window	150 ~ 200 750 ~ 1,500 1500 ~ 3,000	14 ~ 18 70~140 140 ~279
•	HOSPITALS Sickroom, Warehouse Medical Examination room Operating room Emergency Treatmet	100 ~ 200 300 ~ 750 750 ~ 1,500	9 ~ 18 28 ~ 70 70 ~ 140
•	SCHOOLS Auditorium, Indoor Gymnasium, Class room Laboratory, Library, Drafting, room	100 ~ 300 200 ~ 750 500 ~ 1,500	9 ~ 28 18 ~ 70 47 ~ 140

RS Components UK PO Box 99, Corby Northants, NN17 9RS Tel: +44 (0)1536 201234 Fax: +44 (0)1536 405678 Sept-2002